

Model S-265 Scoop

The **Model S-265 Scoop Stretcher** (stretcher) is an emergency patient-handling device. It is designed to aid in moving a patient when space is limited or when the patient needs to be moved with little change of body position. Operate the stretcher according to the laws and protocols of the country where it is used. Consult the appropriate authorities for information regarding laws and protocols, and resolve any questions before using the stretcher with a patient.

The stretcher is for professional use by a minimum of two trained operators.



The stretcher frame is constructed in two halves which uncouple, slide under the patient, then recouple for lifting the patient. The stretcher may also be used in a "V" shape when uncoupled at only the foot end.

Other features include a telescoping foot section with locking positions for length adjustment, three handholds on each side of the main frame, and concealed hinges which allow the stretcher to fold for storage.

The Model S-265 stretcher is equipped with a set of three patient restraints.

The stretcher is made from robust aluminium plates and tubes, surface treated by anodization and powder coating respectively and is fully bacterial, fungal, putrid, petrol-oil, stain resistant and easy to clean and disinfect.

Product Specifications

Length open:	1660 mm
Length max:	2013 mm
Length Folded:	1200 mm
Width:	422 mm
Height open:	670 mm
Height Folded:	90 mm
Unit Weight:	9,75 kg
Load Capacity:	159 kg



*Read this manual and
retain for future reference*





1. Adjusting Stretcher Length

Adjust the length of the stretcher to the patient's height **before** uncoupling the halves. This ensures equal adjustment to both halves.

TO LENGTHEN OR SHORTEN THE STRETCHER

1. Move the lock-pin lever on each side of the frame to the unlocked position (Figure 1)
Note: When the stretcher is lying face-up on a flat surface, the locked position is "down" and the unlocked position is "up" (Figure 1)
2. Pull the foot section outward to the desired length, stopping near one of the locking positions located at the holes along the foot-section frame.
3. Return both lock-pin levers to the locked position (Figure 1)
4. Push or pull the foot section a little until it locks into place
5. Make sure both sides are securely locked

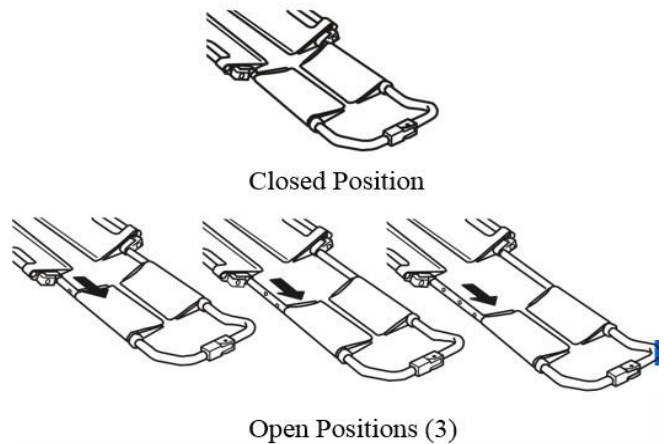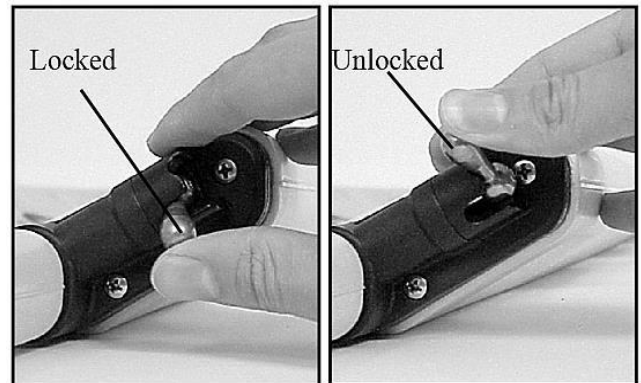


2. Applying the Stretcher

To separate the stretcher halves, use thumbs to press the Twin Safety Lock levers on each end coupling and pull the coupling halves away from each other.



Twin Safety Lock Levers

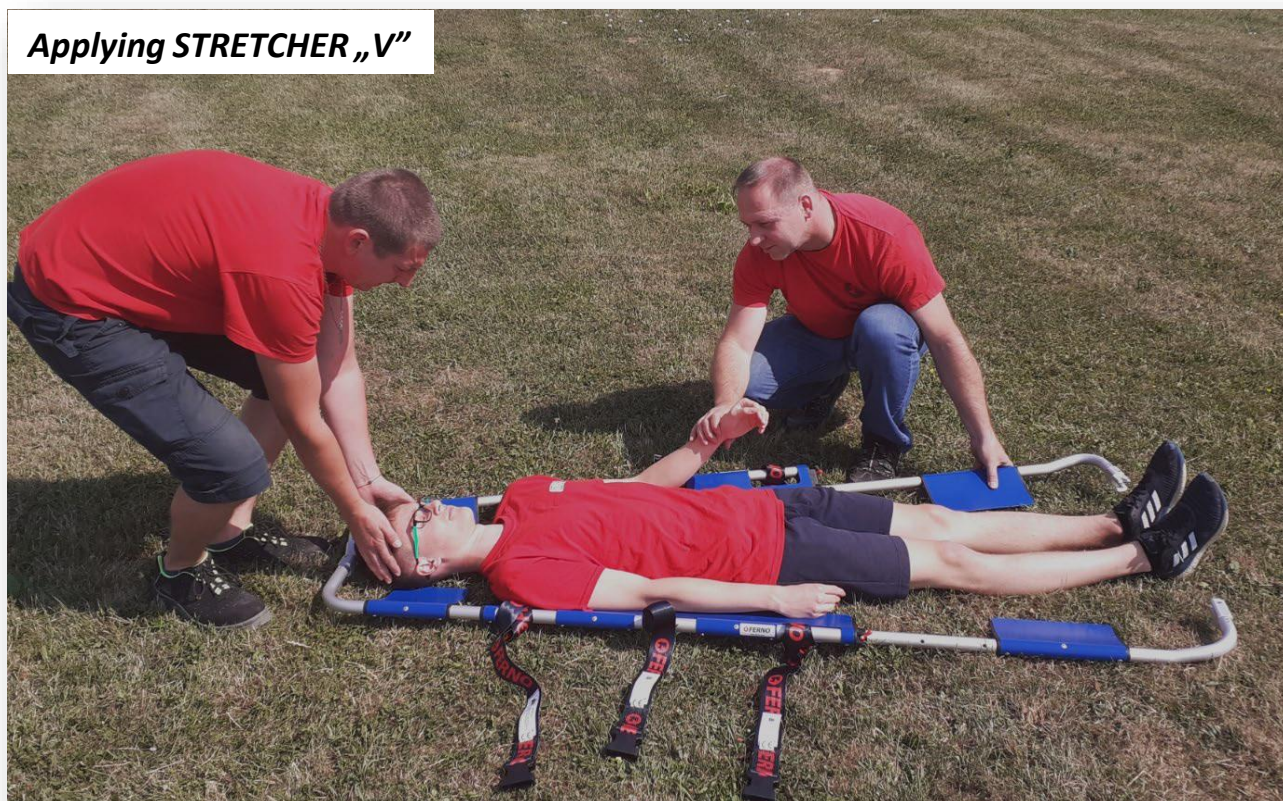

Applying STRETCHER**Applying STRETCHER „V”**

Carrying STRETCHER**3. APPLYING STRETCHER IN A “V”**

Unfold the stretcher if it is folded for storage, and adjust the length (see B Adjusting stretcher length)

1. Unfasten the restraints (if stored on stretcher)
2. Open only the foot-end coupling.
3. Pull the foot end halves of the stretcher apart to form a “V” shape.
4. Position the stretcher with the patient's head at the base of the „V“ (Figure 6)
5. Use locally-approved EMS procedures to work the stretcher inward and under the patient. Work from head to foot until the coupling halves at the foot end meet.


To avoid pinching or pulling the patient's skin, hair, or clothing, use care while working the stretcher halves into place beneath the patient.

4. ATTACHING RESTRAINTS


The Model S-265 Scoop Stretcher includes a set of three two-piece restraints.

To attach a two-piece restraint:

1. Unbuckle the restraint, separating it into two pieces.
2. Pass the looped end of one restraint piece upward through a handle hold opening on stretcher frame.
3. Hold the loop open and thread the buckle of restraint through loop.
4. Pull the webbing through the loop until the loop is snug against stretcher frame.
5. Confirm that all restraints are securely fastened.

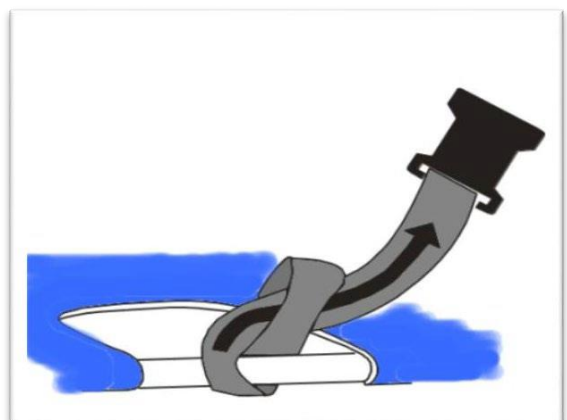

5. USING ADDITIONAL HELP

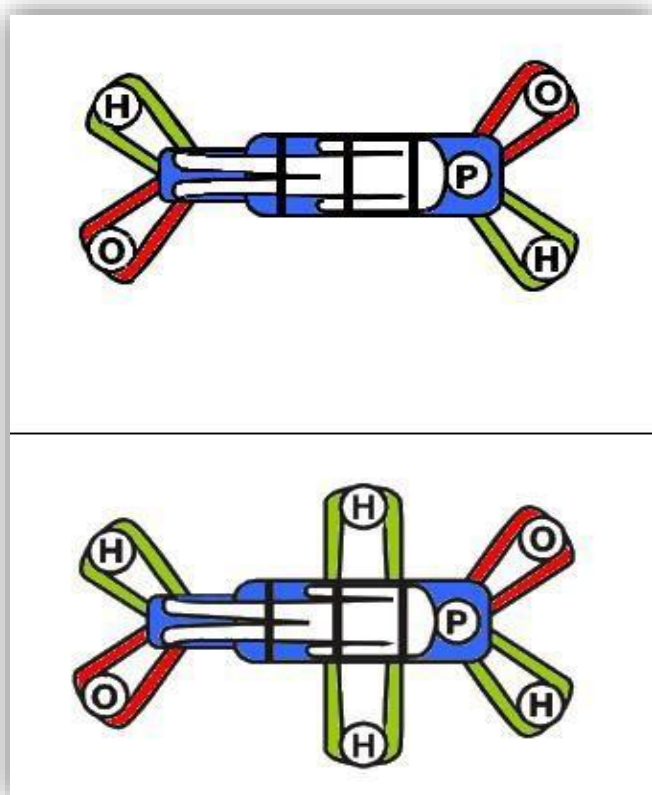


O-Operator H-Helper P-Patient


6. STORING THE STRETCHER

Unfold the stretcher if it is folded for storage, and adjust the length (see B Adjusting stretcher length)

1. Unlock the lock-pin levers on both sides of the stretcher.
2. Fully extend the foot section by pulling it out until the hinges are completely visible.
3. Lift the foot section and fold it over onto the torso panel

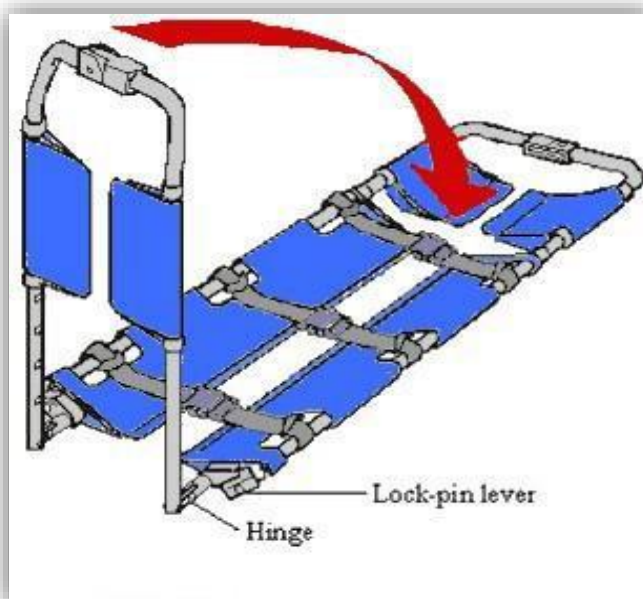


7. STRETCHER COMPONENTS

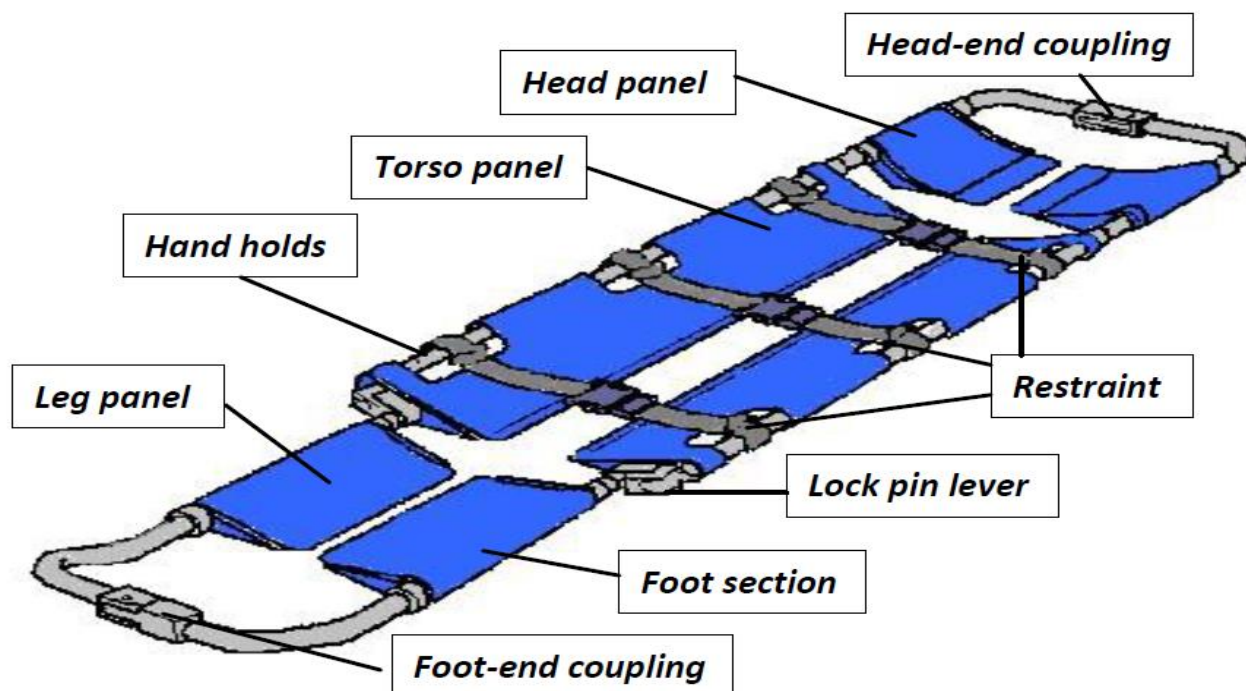

8. Lubricating the Stretcher

- white lithium grease
- SAE 30-weight oil
- Dry-coating Teflon lubricant

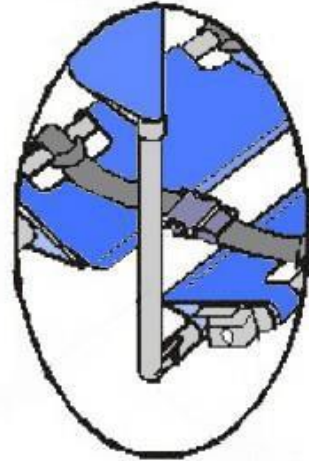

8. Warranty and Service

Standard terms and conditions apply to all sales. A copy is available upon request. These contain full details of warrant terms and do not limit the statutory rights of the customer.

For service, maintenance and any questions regarding this, or any other product, please contact your local distributor.

The CE mark on this product demonstrates conformity with the requirements of the Directive MDR 745/2017 for Medical Devices. The device meets the EN1865-1 requirements.



WARNING

FOR SERVICE AND REPAIR PLEASE REFER TO YOUR SALES AGENT

Improper use of the stretcher can cause injury. Use the stretcher only for the purpose described in this manual.

Untrained operators can cause injury or be injured. Permit only trained personnel to operate the stretcher.

Improper operation can cause injury. Operate the stretcher only as shown in this manual.

An unattended patient can be injured. Stay with the patient at all times.

An unrestrained patient can fall off the stretcher and be injured. Use restraints to secure the patient in the stretcher.

Untrained helpers can cause injury or be injured. Operate and maintain control of the stretcher and direct any helpers.